

7D Focused Ultrasound



SHURINK L4-4.5 and DL4-5 probes are used for focused ultrasound therapy. The L4-4.5 probe is used for the treatment of brain tumors, while the DL4-5 probe is used for the treatment of prostate cancer. Both probes are designed to deliver high-intensity focused ultrasound (HIFU) energy to the target tissue, which can be used to ablate or destroy the tissue. The probes are connected to a 7D Focused Ultrasound system, which allows for precise targeting and monitoring of the treatment area.

FACIAL SCULPTURE

Smaller, more convenient, more accurate, more suitable for facial skin

- 1.5 mm
- 3.0 mm
- 4.5 mm

7D HF HANDLE

More comprehensive, more detailed and more suitable for comprehensive treatment of the body


- MF2
- MF6
- MF9
- MF13
- L4-4.5
- L7-1.5
- L7-3.0



00000000, 00000000 00 000000 0000 000000 00, 00000000 00000000 00000000 0000 000000 000000000000 000000
 000000 0000 00000000 00000000, 000000000000 0000 00 000 000 0000. 000000 000000 000 000000 00000000 000000 000
 00000000 00000000 00000000 0000 00000000 000000 000000 000000 000000 000000 000000, 000000 0-0.5 000 00000000 0000 00000000
 00000000 00 00000000 (SMAS), 0000000000 00000000 00 000 00000, 000000 0000 000000 000 0000 000 000000 00.




EXFU

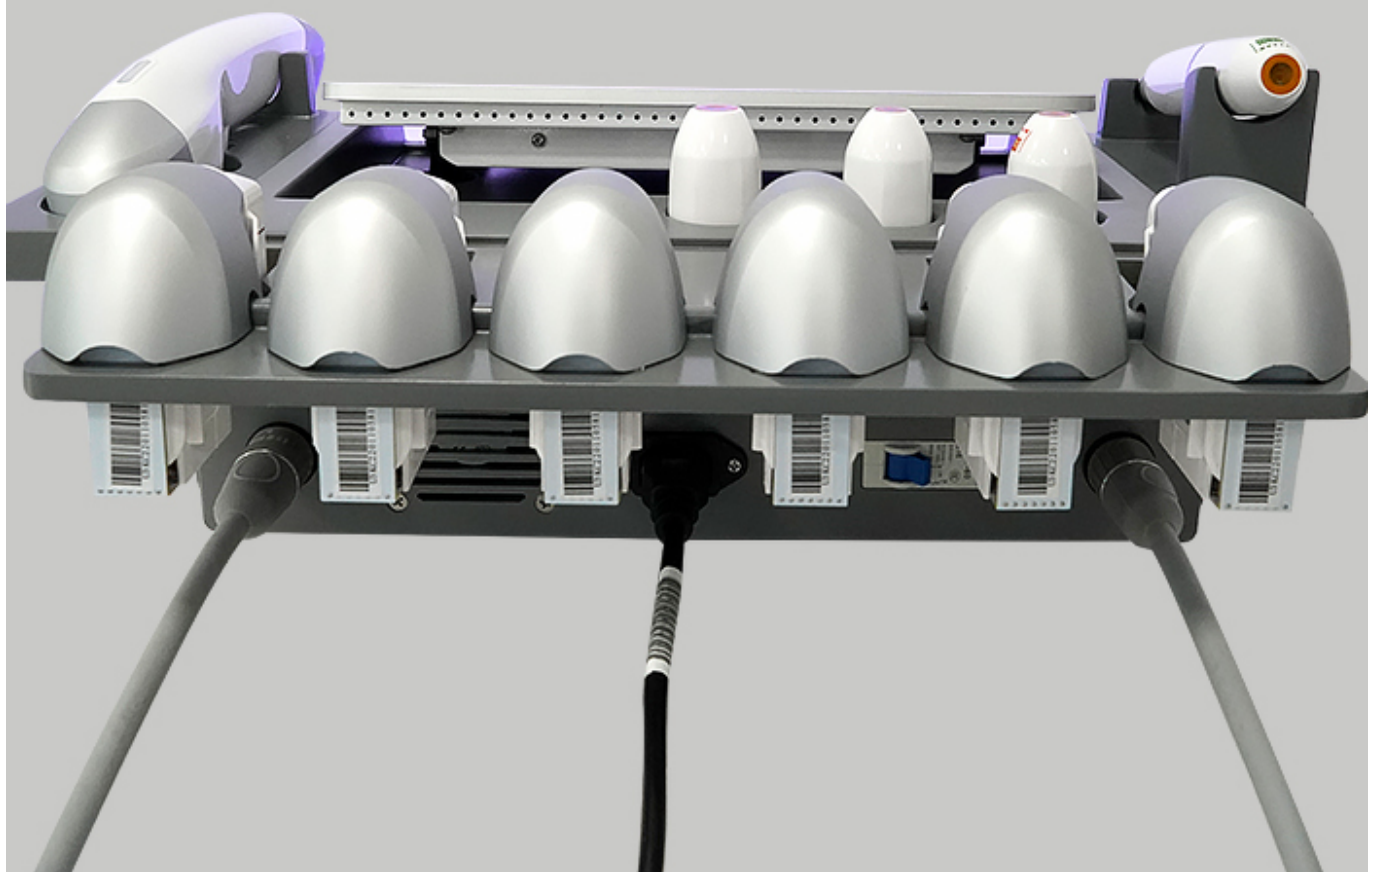


Face Treatment



Body Treatment

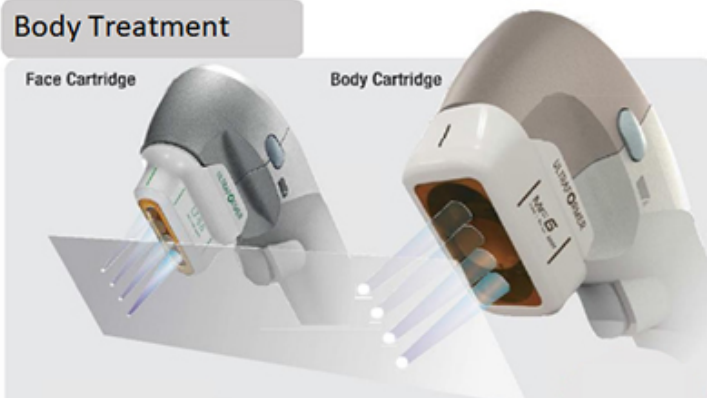

Body Treatment

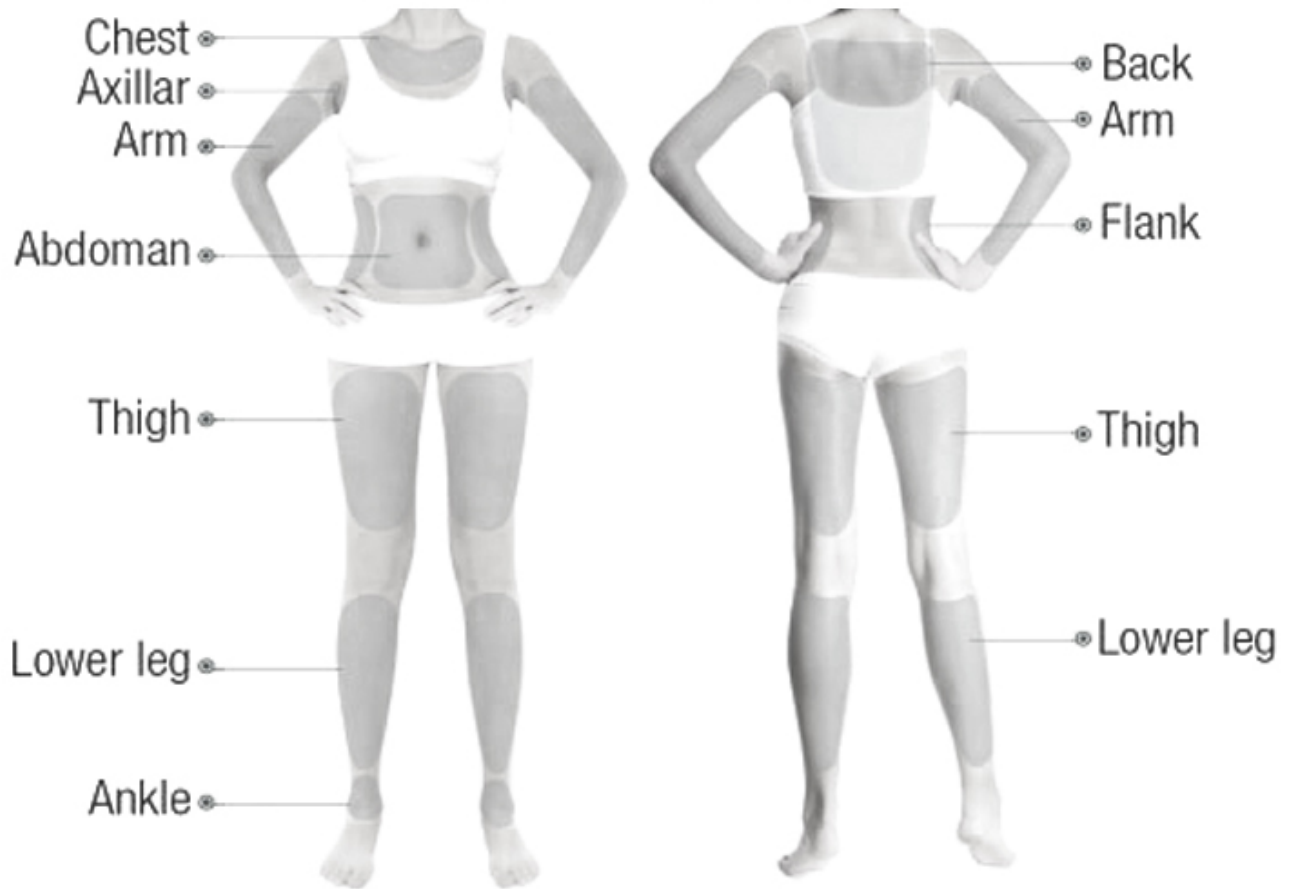

• Treatment Effect •



□□□□	7 □□□□ □□□□ □□□□□□□□□□
□□□□	□□□□ □□□□ □□□□ □□□□□□□□□□

探头	4.5" 3.0" 1.5" : 探头 探头
探头	7D HF: MF2/6/9/13 L4-4.5 L7-1.5 L7-3.0
探头 探头	0.1J-2.5J (0.1J 探头 探头)
探头 探头 探头	1.0" 4.0"
探头 探头	5" 25"
探头	300000 探头 探头
探头 探头	15"
探头	110V-240V, 50/60Hz



1. 探头 探头 探头 探头
 2. 探头 探头 15.6 探头 探头 探头 探头
 3. 探头 探头 6, 探头 探头, 探头/探头
 4. OEM 探头(探头) 探头...
 探头 探头 探头 探头 探头 探头!